

A Multisensory System for the Development of Sound Awareness and Speech Production

Kimberly V. Fisher and Barbara J. Parker
*Department of Communication Sciences and Disorders
University of Oklahoma Health Sciences Center*

The Multisensory Sound Lab (Oval Window Audio) is educational technology developed for use by groups of children who are deaf or hearing impaired. It provides simultaneous visual, tactile, and auditory information in response to acoustic inputs. A sound-sensitive floor that is large enough to seat 15 children provides the vibrotactile information. Frequency information may be transposed downward as much as 2 octaves in order to enhance the vibrotactile and auditory experience. Visual feedback includes colorful line spectra, kaleidoscope patterns, and a frequency sensitive light tower. The amount and type of multisensory reinforcements can be adjusted by the user. Sound Lab applications might include auditory detection, sustained voice production, or speech sound production activities. This paper describes applications, advantages, and limitations of the Multisensory Sound Lab for use in a clinical setting.

Traditionally, auditory skills have been described as a multi-stage process (Erber, 1982). First, detection or attention to sound is required. That is, only recognition of the presence or absence of sound is necessary. No categorization or meaning is linked to the sound. The second stage is discrimination between sounds. Differences among speech sounds may be very small, yet carry a great deal of information, such as the simple addition of /s/ to the end of a word. The third step, identification, requires the listener to understand that a sound is “different” and also to attach some memory to the sound. Comprehension, the final stage,

Kimberly V. Fisher is Assistant Professor, Department of Communication Sciences and Disorders, University of Oklahoma Health Sciences Center, Oklahoma City, Oklahoma. Barbara J. Parker, Director of Audiology, is currently affiliated with Providence Speech and Hearing Center, Orange, California.

is the most difficult. The linguistic and non-linguistic coding that is embedded in the acoustic signals must be understood (Condon & Sander, 1974; Engle, 1973; Hirsh, 1940).

More recently, Aslin and Smith (1988) proposed a developmental model in which sensory skills emerge sequentially in three levels: the sensory/primitive level, perceptual representation level, and the cognitive/linguistic level. Moeller and Carney (1993) further describe how normal auditory/perceptual skills may develop within this model. First, the sensory/primitive level develops as the child's sensory systems change incoming physical signals into a stimulation pattern. In the auditory system, the sensory/primitive level includes sound detection. Next, the child uses the stimulation pattern to form a complex neural code or perceptual representation. This level is thought to address pre-linguistic aspects of speech perception that have been observed in infants (Eilers, Wilson, & Moore, 1977; Kuhl, 1983; Spring & Dale, 1977). The third, and highest level of representation occurs at the cognitive/linguistic level. Auditory comprehension of words and longer utterances appears at this level. Aslin and Smith's developmental model also has been extended to development of speech production in children with hearing impairments and children receiving cochlear implants (Carney et al, 1993; Moeller & Carney, 1993). Helping children who are hearing impaired function successfully from sensory/primitive throughout linguistic stages is important for the development of speech perception and production.

A number of aural rehabilitation programs can be used to address auditory skills described in traditional and/or developmental approaches (Erber, 1982; Shea, 1992; Stout & Windle, 1992). Where appropriate, such programs make use of combined tactile, visual, and auditory information to help people learn to detect, discriminate, identify, and comprehend speech. Further, recent reports suggest that the use of multi-modality stimulation (visual, auditory, and tactile) may provide better results than that observed with only one or two sensory modalities (Carney & Beachler, 1986; Carney, Durkel, & Beachler, 1981; Pratt, Heintzelman, & Deming, 1993; Robbins, Osberger, Miyamoto, Renshaw, & Carney, 1988).

Technologies also have been developed to provide immediate multisensory feedback for speech production. When used to assist individuals with hearing impairment, devices are intended to provide the speaker with additional visual or tactile information related to their own motor or acoustic speech events (Fletcher, 1989). In some cases these include computer-based systems (Osberger, Moeller, Kroese, & Lippmann, 1981; Pratt et al., 1993). Most of the currently available systems provide simultaneous feedback in one or two sensory modalities.

The purpose of this report is to describe trial applications of the Multisensory Sound Lab¹ (Oval Window Audio). The system, originally designed for use by

¹Multisensory Sound Lab is a product of Oval Window Audio. Information about the laboratory

groups of children who are deaf, provides simultaneous sensory stimulation through visual, tactile, and auditory modes. Educational applications representing a variety of primitive and linguistic levels of intervention are provided. The examples include both single-user as well as group intervention methods.

The Technology

The Multisensory Sound Lab is an audio system that amplifies sound through loudspeakers and simultaneously transforms sound into floor vibrations that can be felt through the body and seen through a variety of visual displays. Typical components of the system are shown in Figure 1. The components can include a vibrotactile floor, spectrum analyzer (Visualizer), frequency sensitive light tower (Luma Light), laser light display, tone generator, oscilloscope, audio speakers, and induction loop assistive listening systems for the hearing impaired. Multiple sound sources such as microphones, audio cassette, CD, or VCR signals provide input to the system. Electronic musical instruments and games are especially well suited to the system. For example, battery-powered sound games (e.g., "Simon"), synthesizers (e.g., electronic keyboards and drum sets), an electronic stethoscope, and an electric bass guitar often are used with the Sound Lab.

The sound floor (see Figure 1a) is comprised of nine interlocking modular panels, each of which covers a 16 ft² (1.5 m²) area. (Figure 1 includes only four panels in order to conserve space.) Once assembled, the floor covers an area up to 144 ft² (13.37 m²). The vibrotactile floor is driven by two loudspeakers that are coupled to the corners of the floor area (see Figure 1b). People sitting or standing on the floor will perceive sound as vibrations. High frequency sounds that are outside the floor's 20 Hz - 500 Hz range may be transposed downward as much as 2 octaves in order to enhance the vibrotactile experience. Two loudspeakers (in addition to those that drive the floor) are provided so that users have greater control over audio listening levels (see Figure 1c).

The Visualizer (see Figure 1d) is a $\frac{1}{2}$ octave spectrum analyzer (8 kHz full scale) that displays harmonic content as colorful vertical bars on a television monitor. The type of display is controlled from a keyboard (see Figure 1e). Spectral information is displayed in real time. The system does not provide for data storage, but instantaneous spectral peaks can be captured and held temporarily on the monitor screen. Harmonic content also may be displayed in colorful kaleidoscope patterns (see Figure 2), a feature useful for small children. The patterns are sensitive to both the frequency and periodicity of signals, similar to lissajous figures created when sine wave voltages of various amplitude and phase relationships are applied to the X and Y modes of a cathode-ray oscilloscope. Quasi-periodic signals, such as vowels, create an open circle or square pattern (see Figure 2a). Quasi-random signals, such as fricatives, result in filled or

can be obtained from Norman Lederman, Director, Oval Window Audio, 33 Wildflower Ct., Nederland, CO 80446; Voice, Fax, or TDD (303) 447-3607.

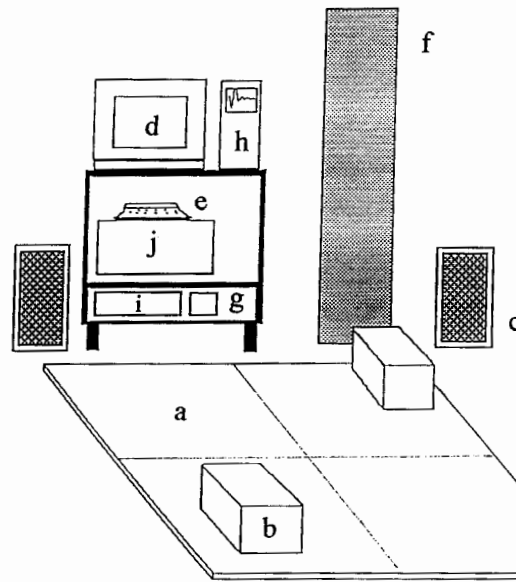


Figure 1. Example components of the Multisensory Sound Lab include: (a) sound floor, (b) floor loudspeakers, (c) audio loudspeakers, (d) Visualizer, (e) keyboard, (f) Luma Sound Light, (g) light controls, (h) oscilloscope, (i) cassette tape player, and (j) control box. Sound toys and a laser light display (not shown) also are available with the system.

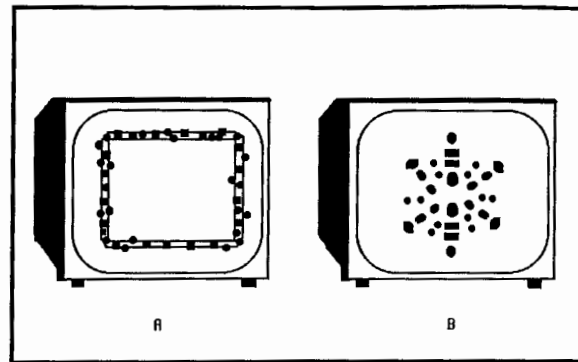


Figure 2. The kaleidoscope display produced by the Visualizer for a vowel and fricative, respectively.

snowflake patterns (see Figure 2b). Larger figures correspond to lower frequencies; smaller figures correspond to higher frequencies.

Another visual display is the Luma Sound Light (see Figure 1f). It is a 7 ft (2.13 m)-tall column made of translucent plastic that contains three banks of color lights. The color lights respond to different frequency bands and sound intensities. The sensitivity of each color bank can be adjusted independently so that the user can modify the relative amounts of visual feedback for different frequency bands (light controls, see Figure 1g). With the ambient lighting dimmed, the Luma Sound Light provides a larger-than-life, colorful, and attention-gaining reinforcement. A nonstorage oscilloscope (see Figure 1h) also is included to allow for waveform display and calibration.

The Sound Lab includes separate amplifiers for up to five simultaneous external inputs. In our system, one of these amplifiers is dedicated to a cassette tape player (see Figure 1i). Additional amplifiers provide for attenuation of floor vibration and light sensitivity separate from the external input gains. This allows the attenuation or amplification of visual reinforcement to be independent from the acoustic signal conditioning. For example, a clinician can gradually attenuate the amount of visual and vibrotactile reinforcement while maintaining the necessary sound audibility.

Because the Lab sustains use by many student clinicians, outside personnel, and groups of clients, it is, by necessity, sturdy and easy to use. The signal inputs, control electronics, amplifiers, signal generator, and frequency counter are housed within a single box that is covered with Velcro (see Figure 1j). Small peripheral toys and a sound level meter adhere to the box with Velcro for ready availability. For ease of use, red "don't touch" stickers are used to mark the default settings for most applications. Any button or knob without a sticker is free for manipulation by the user. An informal survey of our student clinicians and clinical faculty members revealed that about 45 min were needed to become proficient in operating the equipment and accessory devices. In 2 years of operation we have experienced only one minor equipment failure.

EXAMPLE APPLICATIONS

Application 1: Sound Detection

A nonverbal 2 year, 2-month-old female with bilateral moderate to severe hearing loss was introduced to the Sound Lab. She was accompanied by her mother and clinician. A primary concern was nonresponsiveness to sound. The child wore binaural hearing aids and was seated on the sound floor with the assistance of her mother. Environmental lights were dimmed to minimize distraction and maximize the visual impact of the Luma Sound Light. Sound stimuli included the mother's voice, an electronic bass drumbeat, and a battery-powered toy cow that "moored." The mother's voice and cow's moo were directed to the system

with two microphones, and transposed downward to maximize the vibrotactile sensation on the floor. Each sound was presented at suprathreshold level and with maximum feedback from the floor and Luma Light. The clinician monitored the child's responses to the paired sound and multisensory reinforcements. Head turns, pointing, and floor touching were interpreted as positive responses. After consistent responses to the paired stimuli, the feedback from the floor and Luma Light gradually were reduced.

When sound was first presented, the child immediately lay upon the floor, palms down, in front of the Luma Light. This behavior presumably increased the child's sensation of floor vibration, although there are relatively few systematic studies of vibrotactile sensitivity on areas such as the thighs, torso, and chest. Within a 20-min period, however, the child responded consistently to the cow's moo and her mother's voice without visual or vibrotactile feedback. With no simultaneous multisensory stimulation, occasionally the child evidenced frustration and pointed at the unlit Luma Light when sound was presented. In this case, the clinician simply flashed the Luma Light as reinforcement for correct detection of sound.

Application 2: Sound Comprehension

Five kindergartners and first graders who are moderately to severely hearing impaired were referred for trial classroom activities in the Sound Lab. One behavioral objective for these children was naming (oral or manual) of soft and loud sounds. The children were accompanied by two teacher assistants and a speech-language pathologist. All were seated in a circle in front of the Luma Light and television monitor. All children wore binaural hearing aids and were reported to benefit from their use. The teacher assistants indicated that none of the children consistently identified both loud and soft sounds in the regular classroom.

The clinician alternately placed hard or soft objects in a can and shook the can in front of a microphone that provided input to the Sound Lab. Objects and amplifier gains were selected such that hard objects resulted in visual, auditory, and vibrotactile feedback. Soft objects, however, resulted in only auditory feedback. The auditory signal of soft sounds also was somewhat attenuated, though audible, for the children. Objects included were marbles, pennies, hard plastic toy figurines, wet sponge pieces, crumpled paper balls, and foam squares. The can was passed among the children who each shook the can in turn and would sign and/or vocalize the concepts "loud" or "soft."

After children were familiar with the sound system and identification task, the clinician would alternately place hard or soft objects in the can. She then gave an individual student the opportunity to shake the can and identify the sound as "loud" or "soft." Other children would monitor the accuracy of their peer's answer. Near the end of the activity, the clinician put cotton balls into the can. In

this case, can shaking resulted in no audible sound, and no visual or vibrotactile floor feedback. When faced with this dilemma, children would shake the can vigorously while scrutinizing the possible sources for feedback (floor, light, speakers). After several attempts, they would shrug their shoulders or demand to see if there was anything in the can. After 15 min with the activity, one child discovered that she could make soft or loud sounds with the same object by changing the vigor with which she shook the can. Other children imitated this experimenting behavior. In the regular classroom, the teacher and children subsequently completed a similar activity using auditory trainers without the additional vibrotactile or visual feedback.

Application 3: Gross Vocalization

A 5-year-old male who is severely hearing impaired was referred for trial activities in the Sound Lab. A primary concern was his inability to maintain voicing. Clinicians and teachers had encouraged the child to place his hand over the larynx in order to tactually sense voice vibrations, a process that yielded occasionally successful but inconsistent results. The child was accompanied to the Sound Lab by four peers who are hearing impaired and a classroom teacher. All children wore personal FM systems throughout the activity. Hand-held microphones were used for sound input. Frequency information above 800 Hz was attenuated so that blowing, loud breathing, glottal clicks, voiceless fricatives, and other non-target noises would not trigger visual or vibrotactile feedback. The male client stood in front of the television monitor. Spectral information was displayed in kaleidoscope mode so that the modeled vocalizations made open squares or circles on the screen. Two microphones were passed among the other children who each vocalized in turn and lit the screen. Children were encouraged to light the screen as long as possible, thereby prolonging vocalization.

Next a microphone was provided to the client. The clinician elicited a brief instant of voicing from the child using modelling and placement of the child's hand over his larynx. After six attempts with simultaneous visual feedback, the child was able to maintain voicing for several seconds. The vocalization was quickly generalized from sustained vowel-like productions to alternating open-closed syllable-like strings. After having achieved success, the child was unwilling to yield the microphone so that other children could take turns.

Application 4: Articulation

Six third and fourth graders with moderate to severe hearing loss were accompanied to the Sound Lab by their teacher and speech-language pathologist. All children wore personal FM systems for the group activity. One concern for these children was an inability to contrast /s/ and /ʃ/ production. For these children, the Luma Light was calibrated so that the frequency information of /s/ and /ʃ/ (produced in isolation and syllables) triggered differently colored lights. Spectral

feedback from the Visualizer also was used to differentiate the frequency components of the two phonemes. Two microphones provided system input. The audio input was transposed downward approximately 2 octaves, enabling the /f/ production to be sensed minimally through the vibrating floor. Correct /s/ production did not result in floor vibration that could be felt.

First, the clinician modeled correct production of /s/ and /f/ in isolation. Children were shown the vibrotactile and visual differences between the two phonemes. After children could identify the sound from its multisensory feedback, they were encouraged to produce one of the phonemes following the clinician's model. Cued speech was used to maximize the effectiveness of the model. Children took turns, with one of two microphones. All children monitored the production to determine whether it was more like /s/ or /f/.

The children quickly recognized that they must change their production in order to light the correct spectral bars or Luma Light color bank. In some cases, the changes more closely approximated the correct phoneme. Frequently, however, their efforts resulted in more serious distortions than the original attempt. For this reason, it was necessary for the clinician to model and cue each production. Because fricative production is relatively low intensity, it also was necessary for the clinician to maintain close mouth-to-microphone distance for the children. Cloth chairs helped to stabilize the active children and improved the success of the activity. Small clip-on microphones (also available with the Multisensory Sound Lab) could be used with a head mount for activities requiring very close, or highly stable mouth-to-microphone distance.

Application 5: Music Enrichment

A music teacher was concerned that her fourth through sixth grade students who are hearing impaired could not match the meter or tempo of music with body movements or clapping. The teacher had been working on this skill by having students feel the piano sound board or stereo loudspeaker. She reported that these activities had limited success. All children were severely or profoundly hearing impaired and wore binaural hearing aids.

We asked the teacher to select an audio tape that she used in the classroom. In addition, low frequency dominant stimuli (a tape of rap music, and tapes of common folk songs played in cello) were provided. An electronic bass drum and tom-tom rhythm were produced by a synthesizer. The tempo could be adjusted continuously. A heart beat also was transduced using an electronic stethoscope and willing student participant. The cassette tapes, electronic drum beat, and heartbeat provided the input to the sound system. Stimuli with both predominant beat and low frequency components were considered the easiest to follow rhythmically. The stimuli were presented in order from least to most difficult. The first stimulus was the electronic drum, followed by the heartbeat, rap music, folk songs, and the familiar classroom tape.

Seven students sat on the floor and attempted to match the beat with a foot tap. The teacher assisted some students by patting the basic meter on their shoulders. When each student successfully matched the tempo, a new stimulus was selected. Soon students were familiar with the stimuli, as well as concepts of "basic beat" and "tempo." At this point, each student was given a musical instrument (drum, tambourine, electric bass guitar, cymbal, or chime). The musical sounds were simultaneously directed to the system using external toy inputs and microphones. Gains were adjusted such that high frequency sounds lit the Luma Light, but low frequency sounds created floor vibration. The student instrumentalists were arranged with high frequency sounds near the Luma Light. A conductor was selected from the group to direct the musicians. The conductor could direct their own unique musical piece, or select from the audio-taped stimuli.

Both students and teacher were enthusiastic about the activity. Students were especially interested in the rap music and instruments. However, by the end of the 45-min session, at least 3 of the 7 students remained unsuccessful in their ability to match the tempo even with the additional visual and vibrotactile information. Often children became more interested in their own music making, than in matching the tempo of others. Still, this activity demonstrates the degree to which a creative, musical, auditory experience can be enriched with visual and vibrotactile information.

Summary

Numerous hardware and software products are now available to provide visual and auditory interactive feedback for auditory habilitation or speech-language therapy. Frequently these products are limited in application to a single user for individual therapy or self-instruction. Service delivery, however often involves small group or classroom instruction. In this case, technology that is designed for group use can be cost effective. The Multisensory Sound Lab seems to meet this need. Although there are a wide variety of products that can provide reinforcement or interactive feedback in one or two sensory modalities (e.g., IBM Speechviewer, Kay Visipitch), the Multisensory Sound Lab provides simultaneous visual, auditory, and tactile feedback. This redundancy potentially could help children with a variety of perceptual problems to utilize their sensory strengths.

Clinical intervention that targets gross sound discrimination and identification, or production of speech targets differing in gross duration, intensity, or frequency information is well suited for the Multisensory Sound Lab format. One limitation of the Sound Lab is the relatively poor frequency resolution of the Visualizer. The $\frac{1}{2}$ octave band spectrum, for example, is too broad to clearly demonstrate differences between vowels. The low cost and simple operation of this component, however, make this limitation less serious.

The Multisensory Sound Lab is not immune to problems that plague clinical application of spectral analyses in general. Soft, high-pitch, or hypernasal pho-

nation can produce inadequate or inaccurate visual feedback for the client. The /s/ and /ʃ/ activity described here was limited to gross phoneme approximation in an isolated context because spectral content of fricatives is highly speaker and context dependent (Harris, 1954; Hughes & Halle, 1956). Furthermore, clinicians must evaluate the saliency of visual information provided in the instantaneous spectral content of fricatives. For example, clinicians should expect the noise band limits of /s/ and /ʃ/ to overlap (Strevens, 1960). Also, classification of /s/ distortions from spectral features may not be possible in many cases (Daniloff, Wilcox, & Stephens, 1980). This complexity can decrease the ease with which children extract important information from the visual displays. Fine discrimination and production activities can be addressed using other techniques.

A semi-permanent space should be allocated for the laboratory because the floor is not easily moved after assembly. The modular, 16 ft² (1.48 m²) interlocking floor panels allow flexibility in classroom arrangement. A nine panel, 144 ft² (13.37 m²) floor seats 15 children or 9 adults comfortably. Client groups larger than 15 are seldom seen in our clinic, so the sound floor dimension has not been a limiting factor. Because relatively few products make extensive use of tactile information for learning (with the exception of vibrotactile hearing aids), the vibrating floor seems to be the most innovative component.

The cost of a system ranges from approximately \$3,000.00 to \$15,000.00 and depends upon the variety of components selected by the user. A system similar to the one described here currently lists for \$13,000.00. Individual components may be purchased separately, so the user can add to the laboratory as finances allow. The sound floor is a relatively more expensive component and costs approximately \$395.00 per panel.

Our experience with the Multisensory Sound Lab has been positive. Faculty and students from other universities, private speech-language pathologists, audiologists, and public school personnel often use the lab for a variety of activities. These activities have involved teaching acoustics, speech therapy, vocal hygiene, hearing conservation, music therapy, and deaf education. Multisensory activities may enliven even the easily bored or therapy-weary client. Given access to such versatile technology, the creative clinician and classroom teacher might develop a wide variety of activities that will motivate a variety of clients (Binzer, Gilmore, & Fabry, 1994). Although initially promising, it will be necessary, through systematic study, to demonstrate the efficacy of this format for specific applications before it can be recommended as a therapeutic tool.

ACKNOWLEDGEMENTS

We express our thanks to three anonymous reviewers and Patricia Kricos, PhD for their thoughtful comments. Also, we gratefully acknowledge the technical assistance of Norman Lederman and Barbara Hendricks. Test site multisensory equipment was made available by Oval Window Audio

and the Small Business Innovation Research (SBIR) Program of the U.S. Department of Education. Portions of this paper were presented at the Academy of Rehabilitative Audiology Summer Institute, Snowbird, Utah, June, 1994.

REFERENCES

- Aslin, R.N., & Smith, L.B. (1988). Perceptual development. *Annual Review of Psychology*, 39, 435-473.
- Binzer, S., Gilmore, R.A., & Fabry, D.A. (1994, June). *Current issues in hearing instruments and technology*. Paper presented at the Summer Institute of the Academy of Rehabilitative Audiology, Snowbird, UT.
- Carney, A., Dettman, D., Higgins, M., Johnson, D., Justice, N., Shaner, C., & Wood, S. (1993). *Facilitating listening and speech skills in children with cochlear implants*. Short course presented at the meeting of the American Speech-Language-Hearing Association, Anaheim, CA.
- Carney, A., Durkel, J., & Beachler, C. (1981). An analysis of visual and vibrotactile cue interaction in speech perception. *Journal of the Academy of Rehabilitative Audiology*, 14, 112-124.
- Carney, A.E., & Beachler, C.R. (1986). Vibrotactile perception of suprasegmental features of speech: A comparison of single channel and multi-channel instruments. *Journal of the Acoustical Society of America*, 79, 131-140.
- Condon, W., & Sander, L. (1974). Synchrony demonstrated between movements of the neonate and adult speech. *Child Development*, 45, 456-462.
- Daniiloff, R.G., Wilcox, K., & Stephens, M.K. (1980). An acoustic-articulatory description of children's defective /s/ productions. *Journal of Communication Disorders*, 13, 347-363.
- Eilers, R.E., Wilson, W.R., & Moore, J.M. (1977). Developmental changes in speech discrimination in infancy. *Journal of Speech and Hearing Research*, 20, 766-780.
- Engle, W. (1973). The development from sound to phoneme in child language. In C.A. Ferguson & D.I. Slobin (Eds.), *Studies of child language development* (pp. 9-12). New York: Holt, Rinehart and Winston.
- Erber, N.P. (1982). *Auditory training*. Washington, DC: A.G. Bell Association for the Deaf.
- Fletcher, S. (1989). Visual articulatory training through dynamic orometry. *Volta Review*, 91, 47-64.
- Harris, K.S. (1954). Cues for the identification of the fricatives of American English. *Journal of the Acoustical Society of America*, 26, 952A.
- Hirsh, I.J. (1940). Acoustical bases of speech perception. *Journal of Sound and Vibration*, 27, 111-122.
- Hughes, G.W., & Halle, M. (1956). Spectral properties of fricative consonants. *Journal of the Acoustical Society of America*, 28, 303-310.
- Kuhl, P.K. (1983). Perception of auditory equivalence classes for speech in early infancy. *Infant Behavior and Development*, 6, 263-285.
- Moeller, M.P., & Carney, A.E. (1993). Assessment and intervention with preschool hearing-impaired children. In J.G. Alpiner & P.A. McCarthy (Eds.), *Rehabilitative audiology: Children and adults* (pp. 107-135). Baltimore, MD: Williams & Wilkins.
- Osberger, M.J., Moeller, M., Kroese, J., & Lippmann, R. (1981). Computer-assisted speech training for the hearing impaired. *Journal of the Academy of Rehabilitative Audiology*, 14, 145-158.
- Pratt, S., Heintzelman, A., & Deming, E. (1993). The efficacy of using the IBM SpeechViewer Vowel Accuracy Module to treat young children with hearing impairment. *Journal of Speech and Hearing Research*, 36, 1063-1074.
- Robbins, A., Osberger, M.J., Miyamoto, R., Renshaw, J., & Carney, A. (1988). Longitudinal study of speech perception by children with cochlear implants and tactile aids: Progress report. *Journal of the Academy of Rehabilitative Audiology*, 21, 11-28.

- Shea, B.D. (1992). *Auditory enhancement guide*. Northampton, MA: Clarke School for the Deaf.
- Spring, D., & Dale, P. (1977). Discrimination of linguistic stress in early infancy. *Journal of Speech and Hearing Research*, 20, 224-232.
- Stout, G.G., & Windle, J.V. (1992). *The developmental approach to successful listening II*. Englewood, CO: Resource Point Inc.
- Stevens, P. (1960). Spectra of fricative noise in human speech. *Language and Speech*, 3, 32-49.